

CALIBRATION CERTIFICATE

Total Weighing Solutions Ltd
 Unit 5 Alvis Way, Royal Oak Industrial Estate
 Daventry, NN11 8PG, UK
 www.totalweighing.co.uk
 Tel: 01327 368020


Customer Details	
Name:	WHILTON MILL LTD
Address:	WHILTON LOCKS DAVENTRY NORTHANTS
	NN1 2NH
Contact:	DAN
Telephone:	

Certificate No.	14140
Date of Calibration:	01/12/2020
Next Due:	01/12/2021

Location:	
Department:	
Manufacturer:	DINI ARGEO
Model:	DFWLB-2
Serial No.:	0100482844
Capacity:	600 Kg
Resolution:	0.1
Tolerance:	+/- 3 divs
Calibration Frequency:	YEARLY

Test Weight/Rig Details
Identification No. and Certificate No.
WEIGHT SET: TWS1 - TWS17, D11724 & B12267
CERTIFICATE NUMBER: 8429, 8430, 8431 & 8432
Test weights and equipment are traceable to ISO17025

Linearity / Accuracy Test				
Test Point Kg	As Found Reading	As Found Deviation	Definitive Reading	Definitive Deviation
0	0.0	0.0	0.0	0.0
40	40.0	0.0	120	80.0
120	119.9	-0.1	119.9	-0.1
160	160.0	0.0	160.0	0.0
200	199.9	-0.1	199.9	-0.1

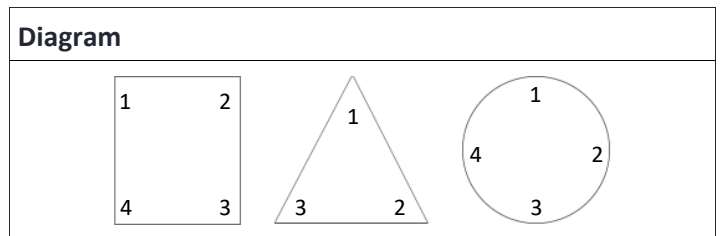

Off Centre Load Test				
Test Point Kg	As Found Reading	As Found Deviation	Definitive Reading	Definitive Deviation
40	40.0	0.0	40.0	0.0
40	40.0	0.0	40.0	0.0
40	39.9	-0.1	39.9	-0.1
40	40.0	0.0	40.0	0.0

Repeatability Test				
Test Point Kg	As Found Reading	As Found Deviation	Definitive Reading	Definitive Deviation
120	120.0	0.0	120.0	0.0
120	120.0	0.0	120.0	0.0
120	120.0	0.0	120.0	0.0

This certificate complies with the United Kingdom Weighing Federation Calibration Code of Practice for non-automatic weighing instruments

Comments	Tolerances
	Unless otherwise agreed, tolerances will be those permitted by current Weights and Measures Regulations for Class III machines as follows:- 0-500 divisions +/- 1div. >501-2000 divisions +/- 2 div >2001 divisions +/- 3div

Technicians Name Ken Goodman

Technicians Signature

